

Fig. 1


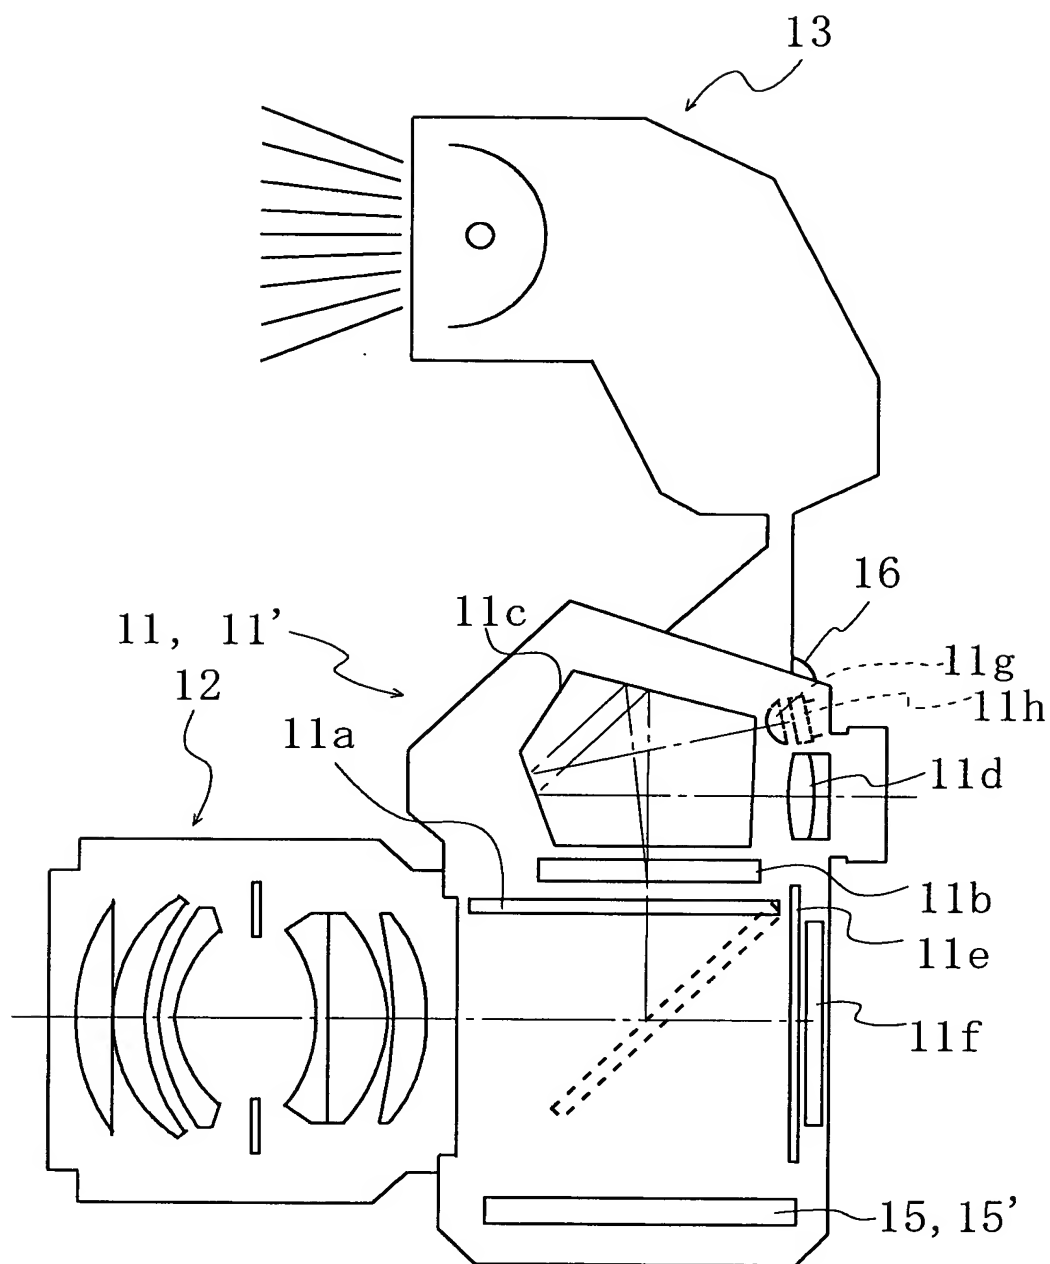


Fig. 2

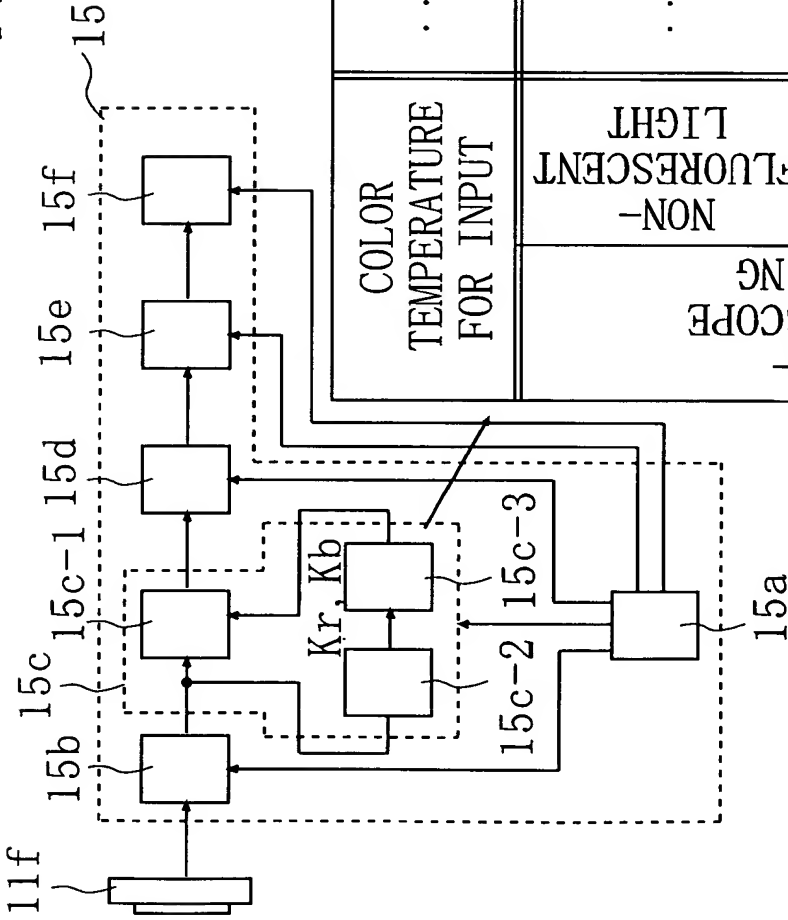

LOOK-UP TABLE

COLOR	...	3900	...	5200	...	6500	...
TEMPERATURE FOR INPUT	...	(Kr, Kb)	...	(Kr, Kb)	...	(Kr, Kb)	...
NON-STROBOSCOPE IMAGING	NON-FLUORESCENT LIGHT	(Kr, Kb)	...	(Kr, Kb)	...	(Kr, Kb)	...
FLUORESCENT LIGHT	...	(Kr, Kb)	...	(Kr, Kb)	...	(Kr, Kb)	...
STROBOSCOPE IMAGING	—	—	—	(Kr, Kb)	...	(Kr, Kb)	—

Fig. 3

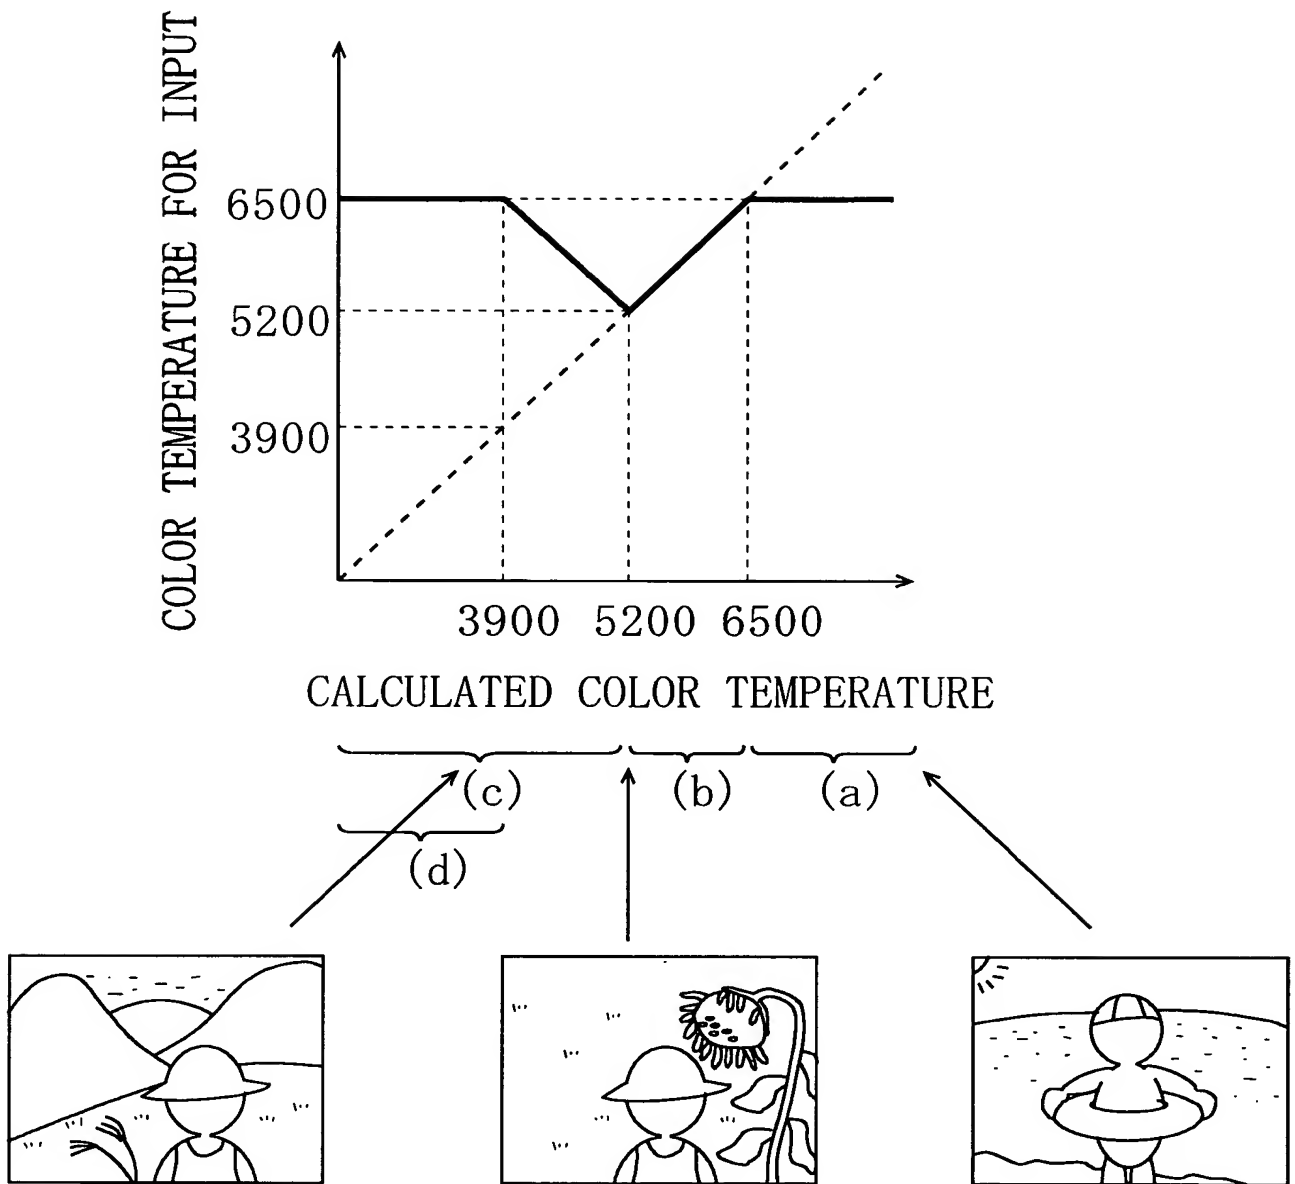


Fig. 4

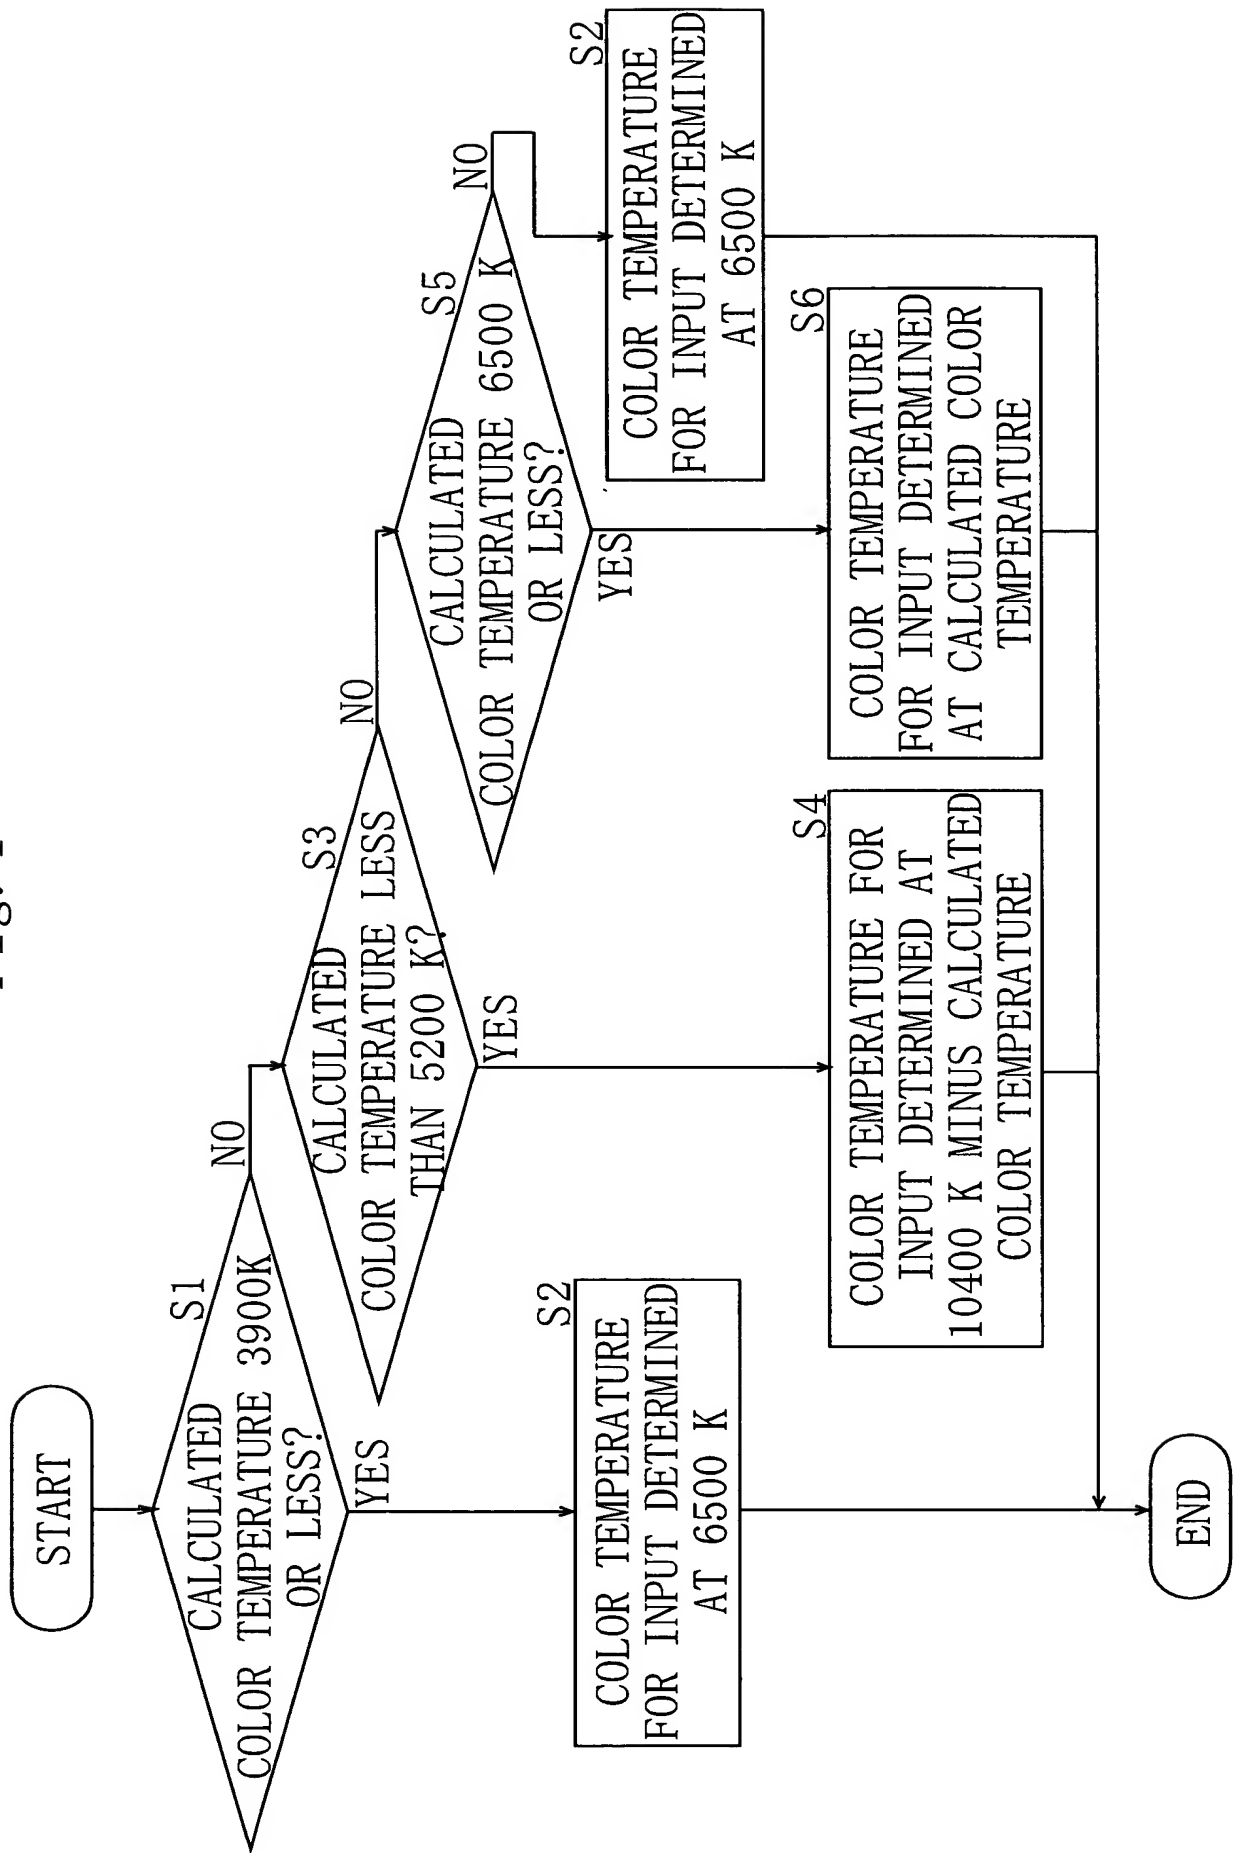


Fig. 5


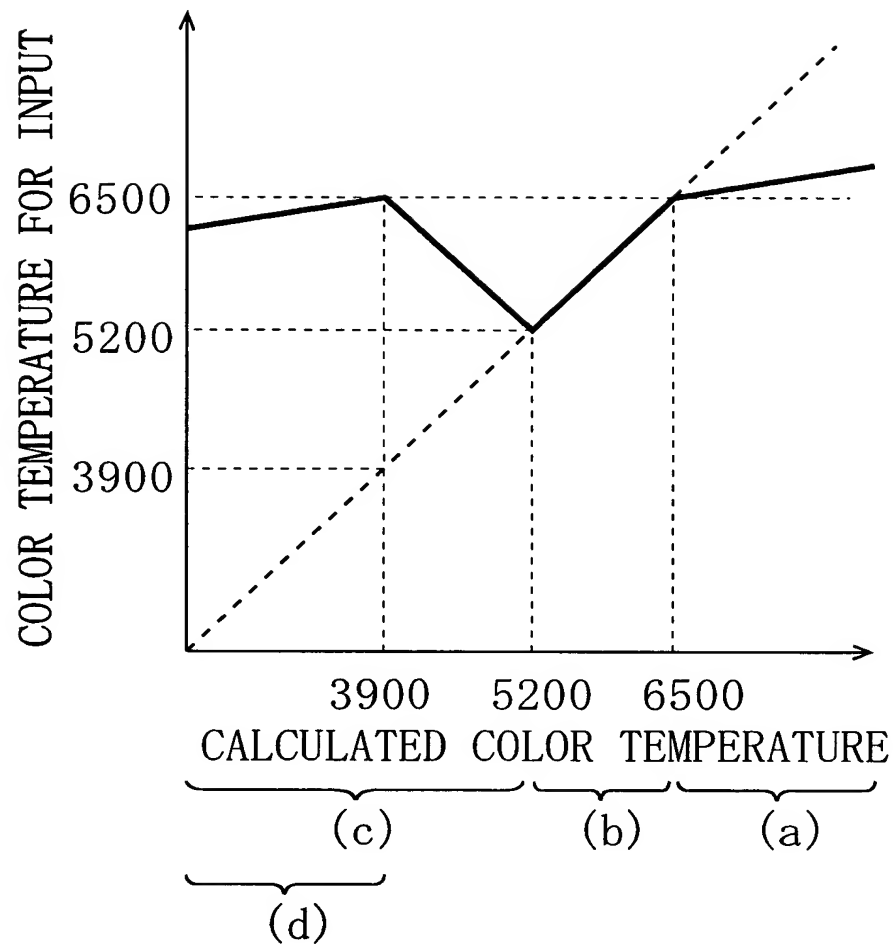


Fig. 6

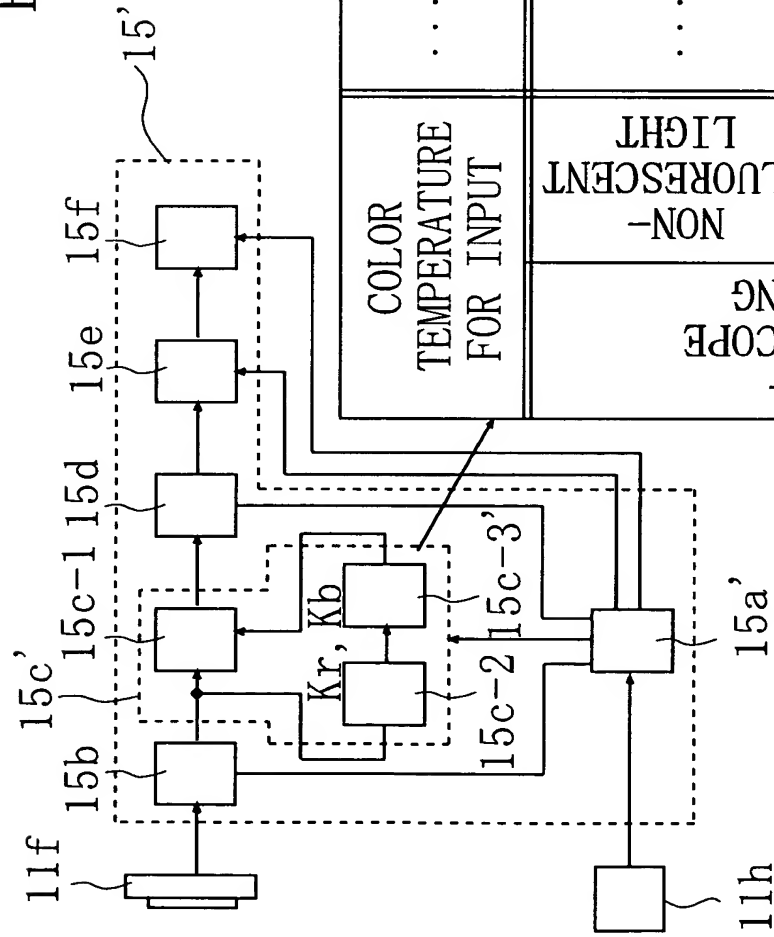


LOOK-UP TABLE

COLOR	...	3900	...	5200	...	6500	...
TEMPERATURE FOR INPUT	...	(Kr, Kb)	...	(Kr, Kb)	...	(Kr, Kb)	...
NON-STROBOSCOPE IMAGING	NON-FLUORESCENT LIGHT	(Kr, Kb)	...	(Kr, Kb)	...	(Kr, Kb)	...
FLUORESCENT LIGHT	...	(Kr, Kb)	...	(Kr, Kb)	...	(Kr, Kb)	...
STROBOSCOPE IMAGING	—	—	—	(Kr, Kb)	...	(Kr, Kb)	—

Fig. 7

(I)

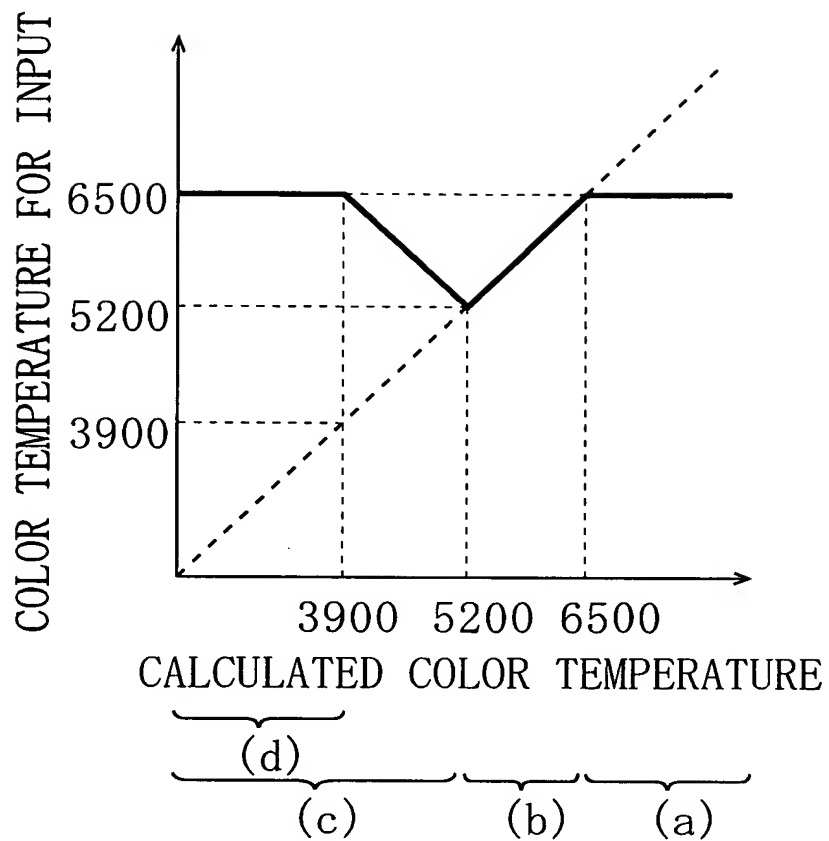

(II)

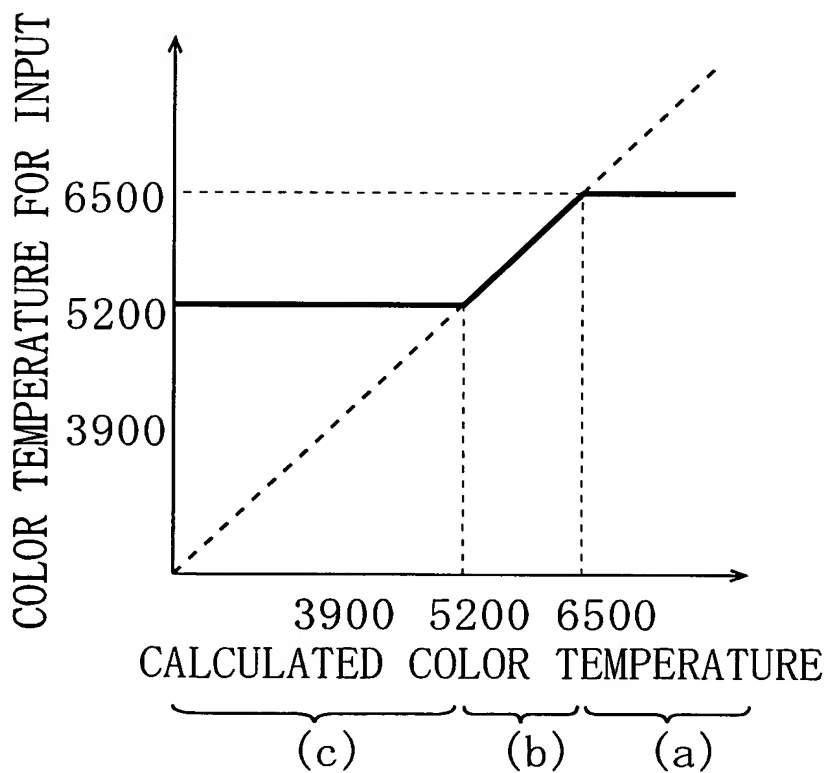


Fig. 8

